





Screenshots for Leica LASX Imaging Software

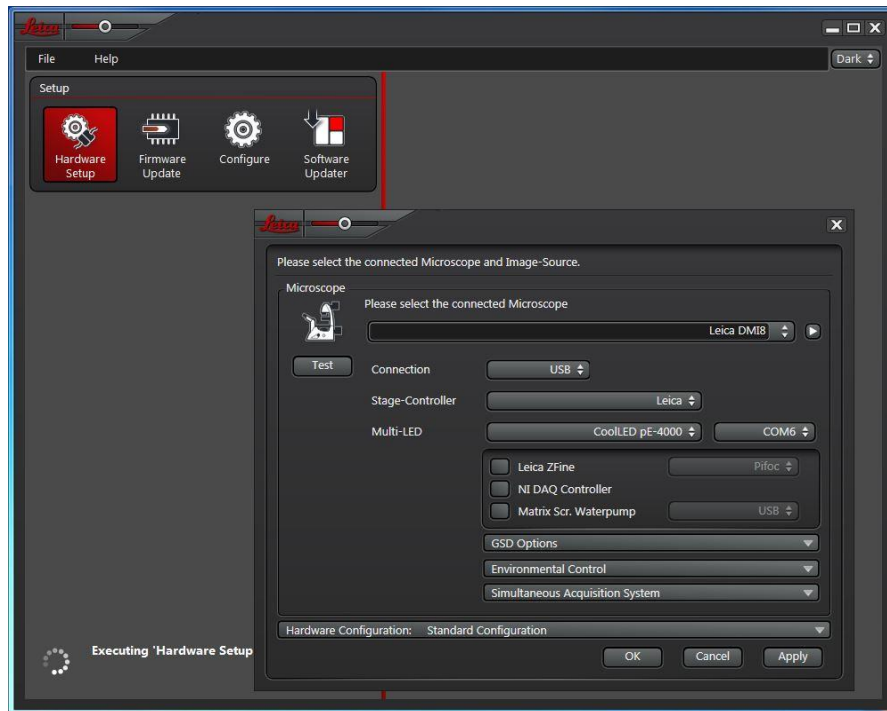

Select CoolLED for use with Leica microscope

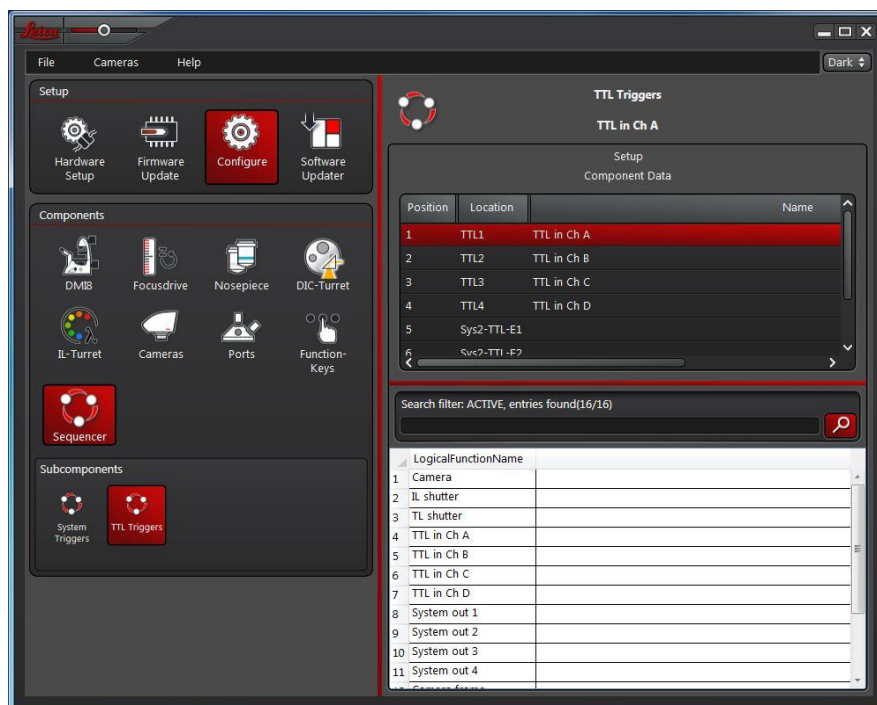

Configure for individual channel control

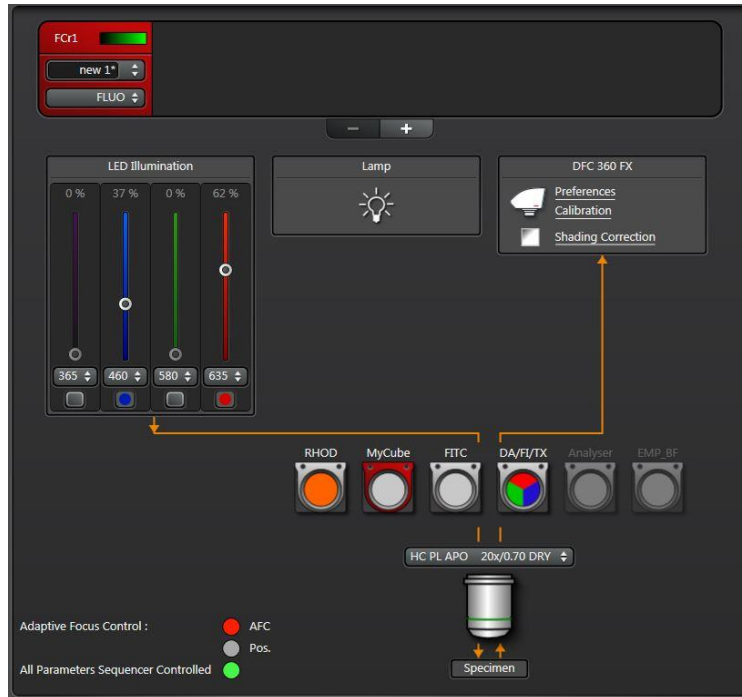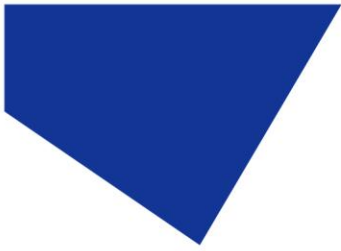

Set intensities for individual channels